


exo

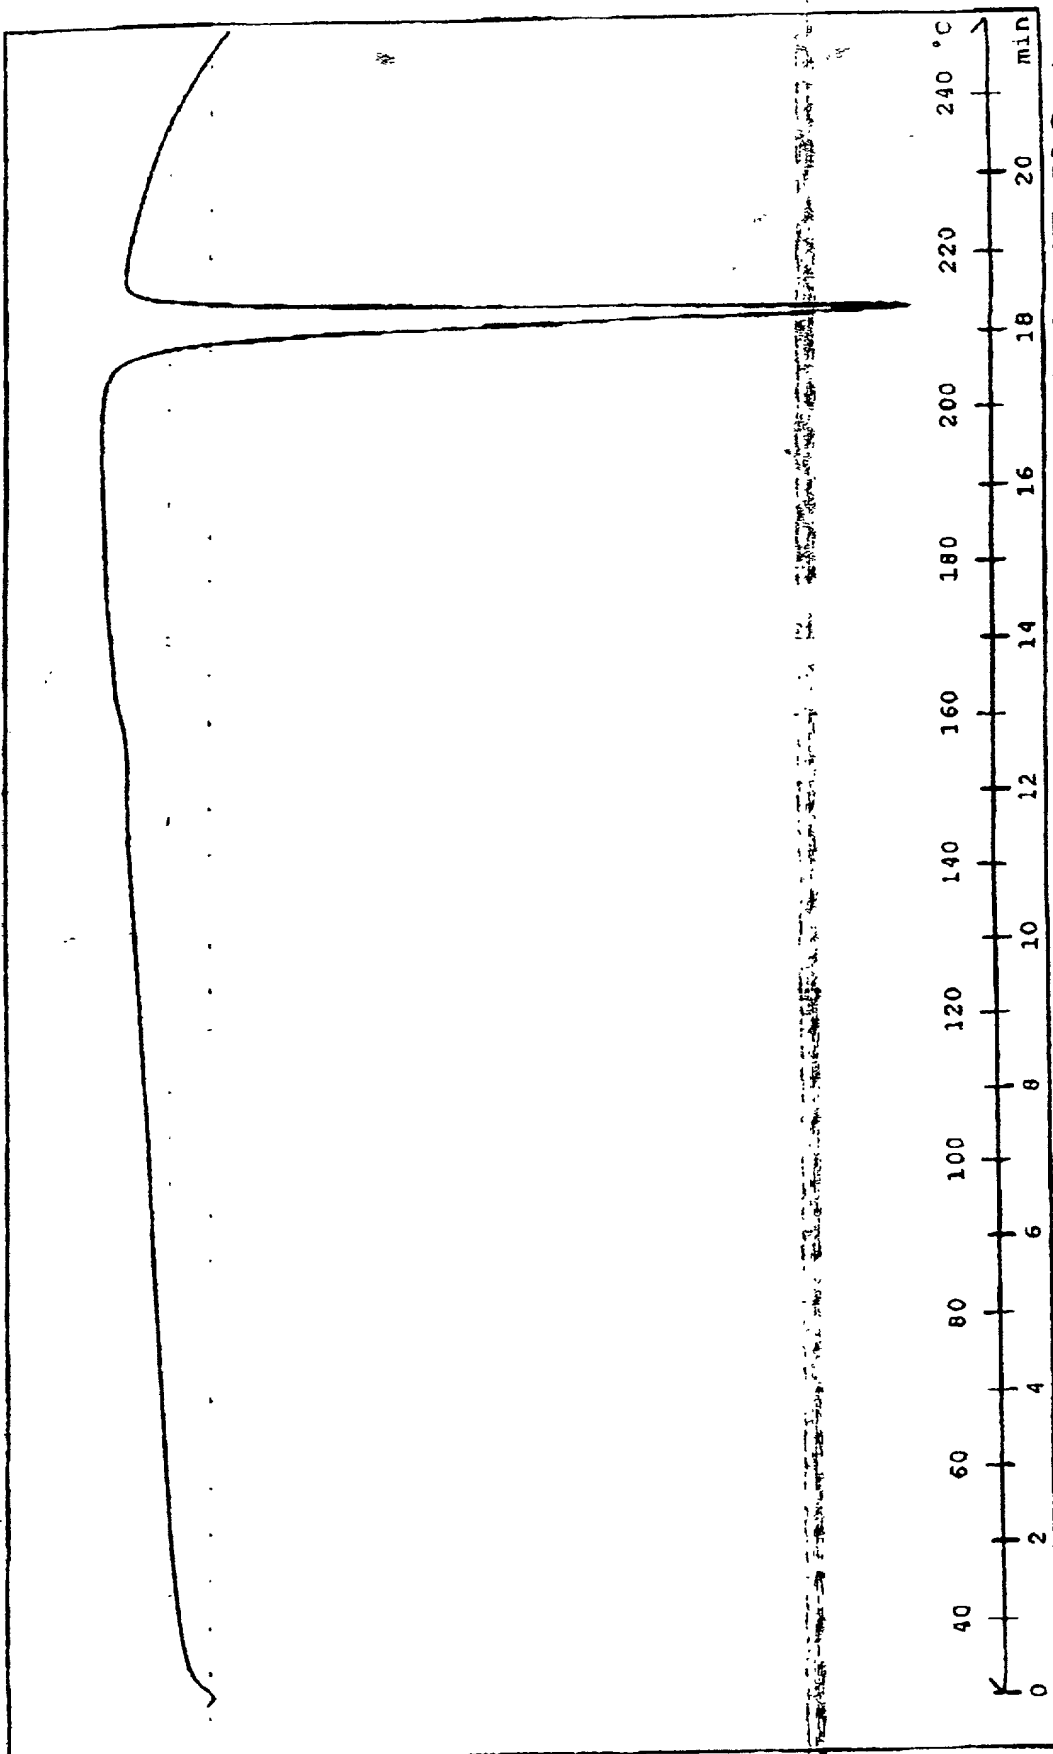

Physical R&D Teva: Shlomo

METTLER TOLEDO STAR® System

Figure 1


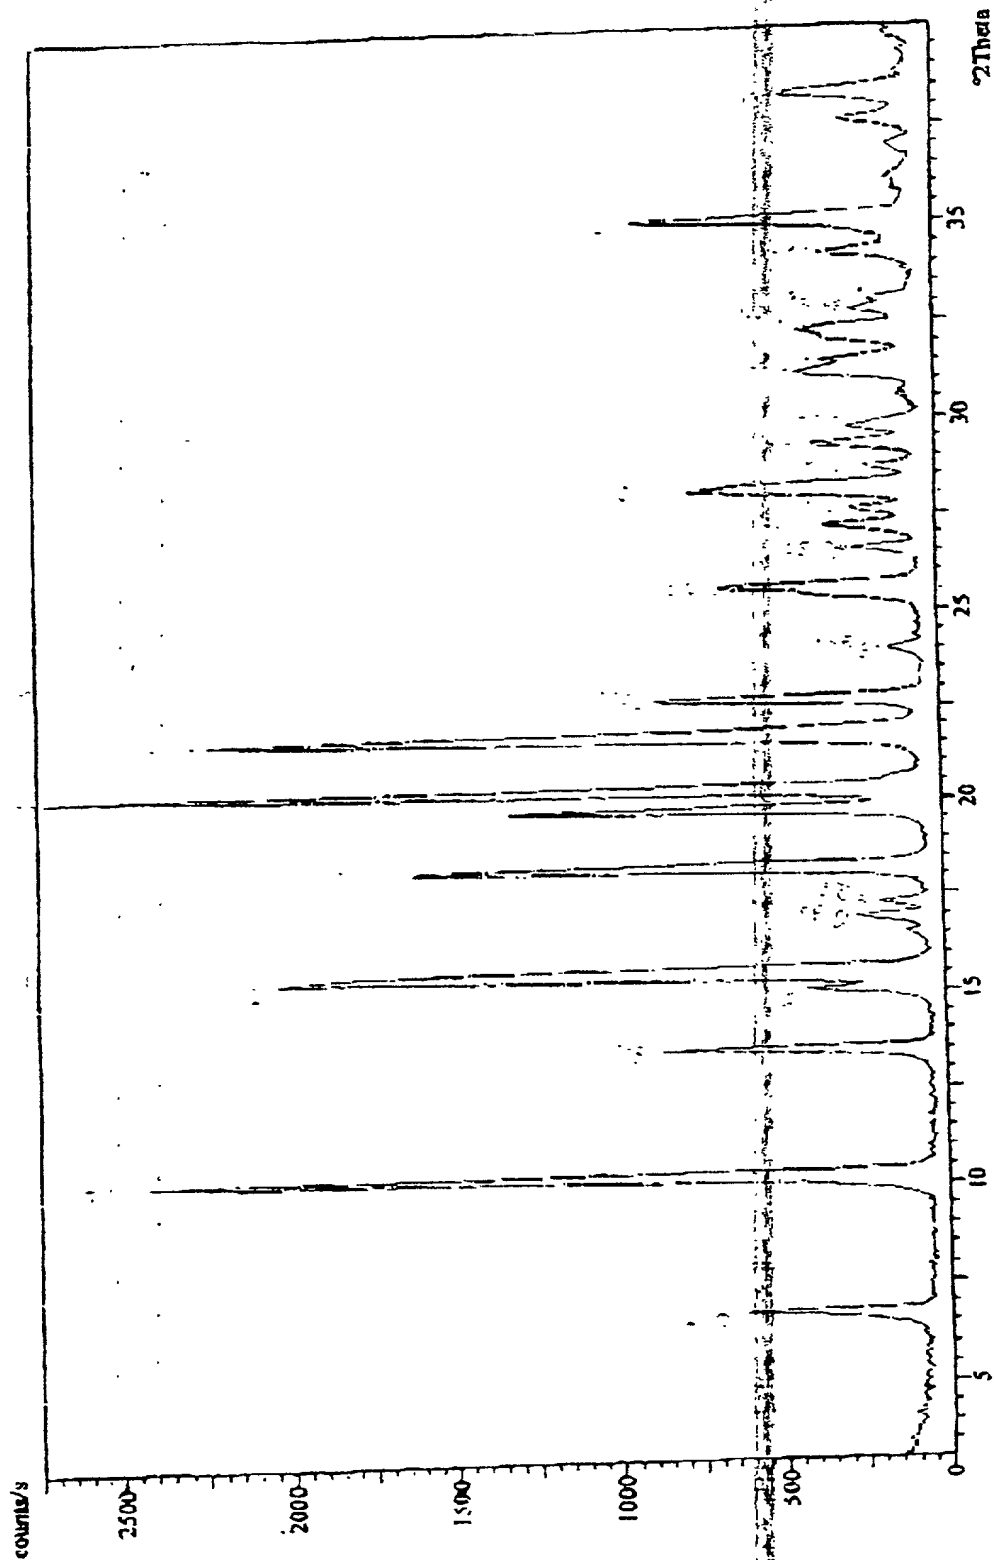


Figure 2

exo

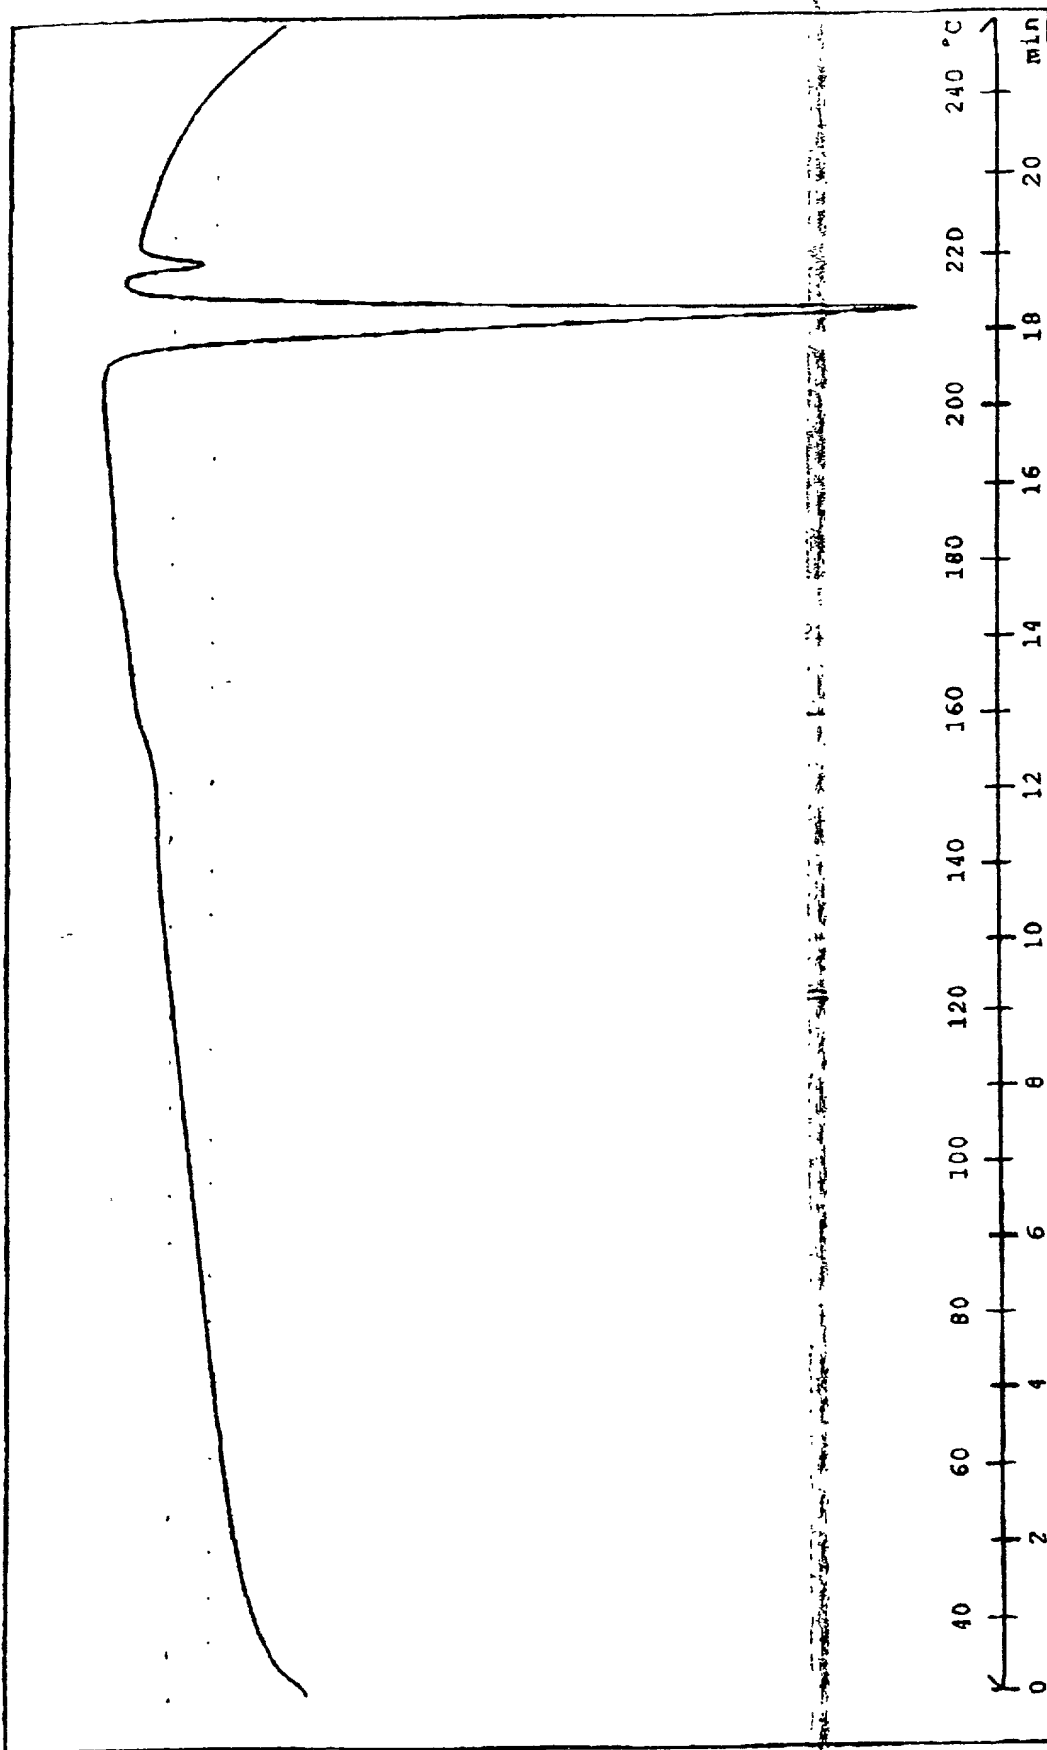

Physical R&D Teva: Shlomo

METTLER TOLEDO STAR° System

Figure 3

TOP OF SHOT

II


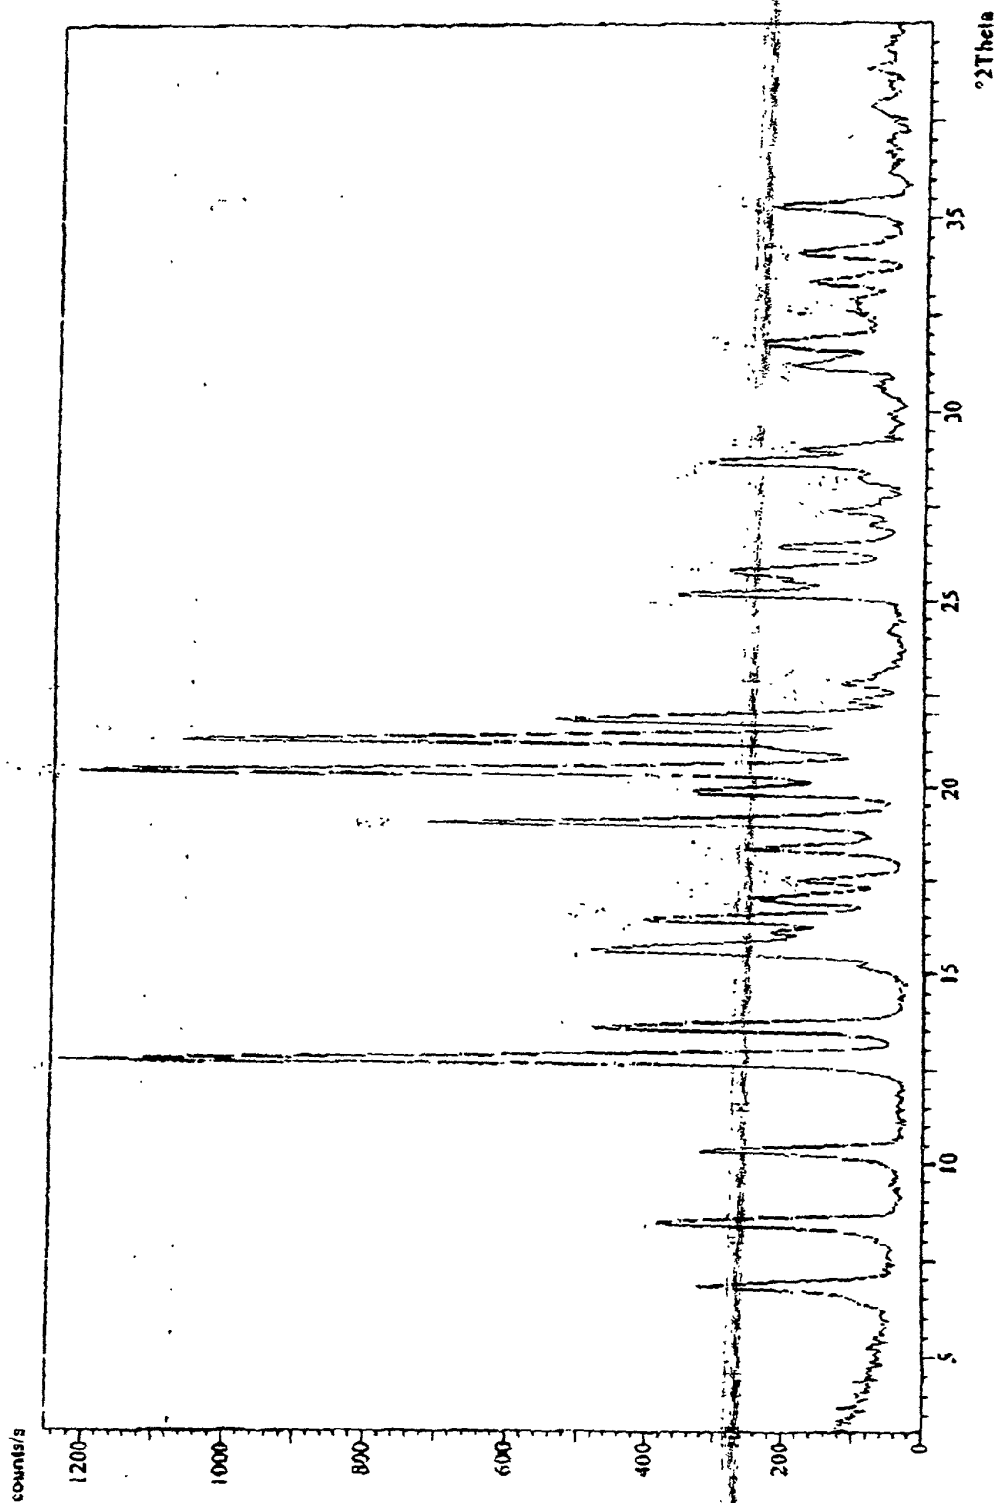


Figure 4

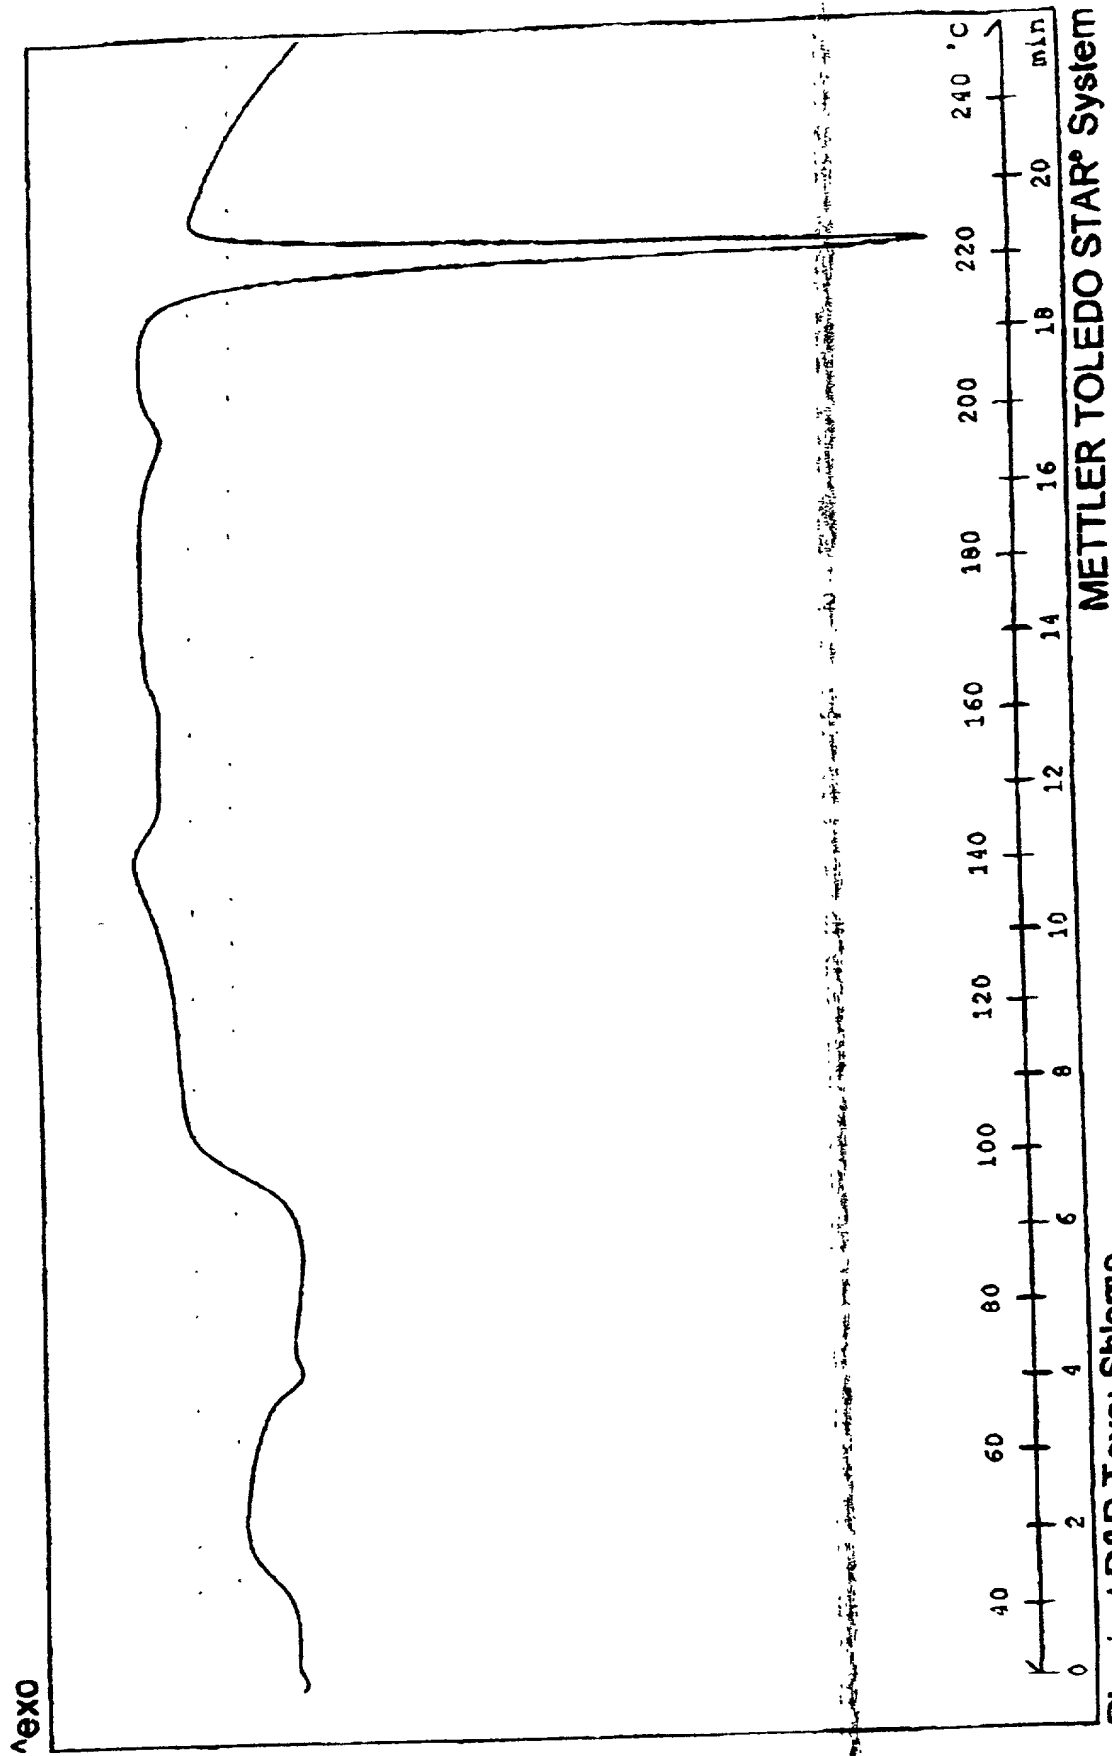

Physical R&D Teva: Shlomo

Figure 5


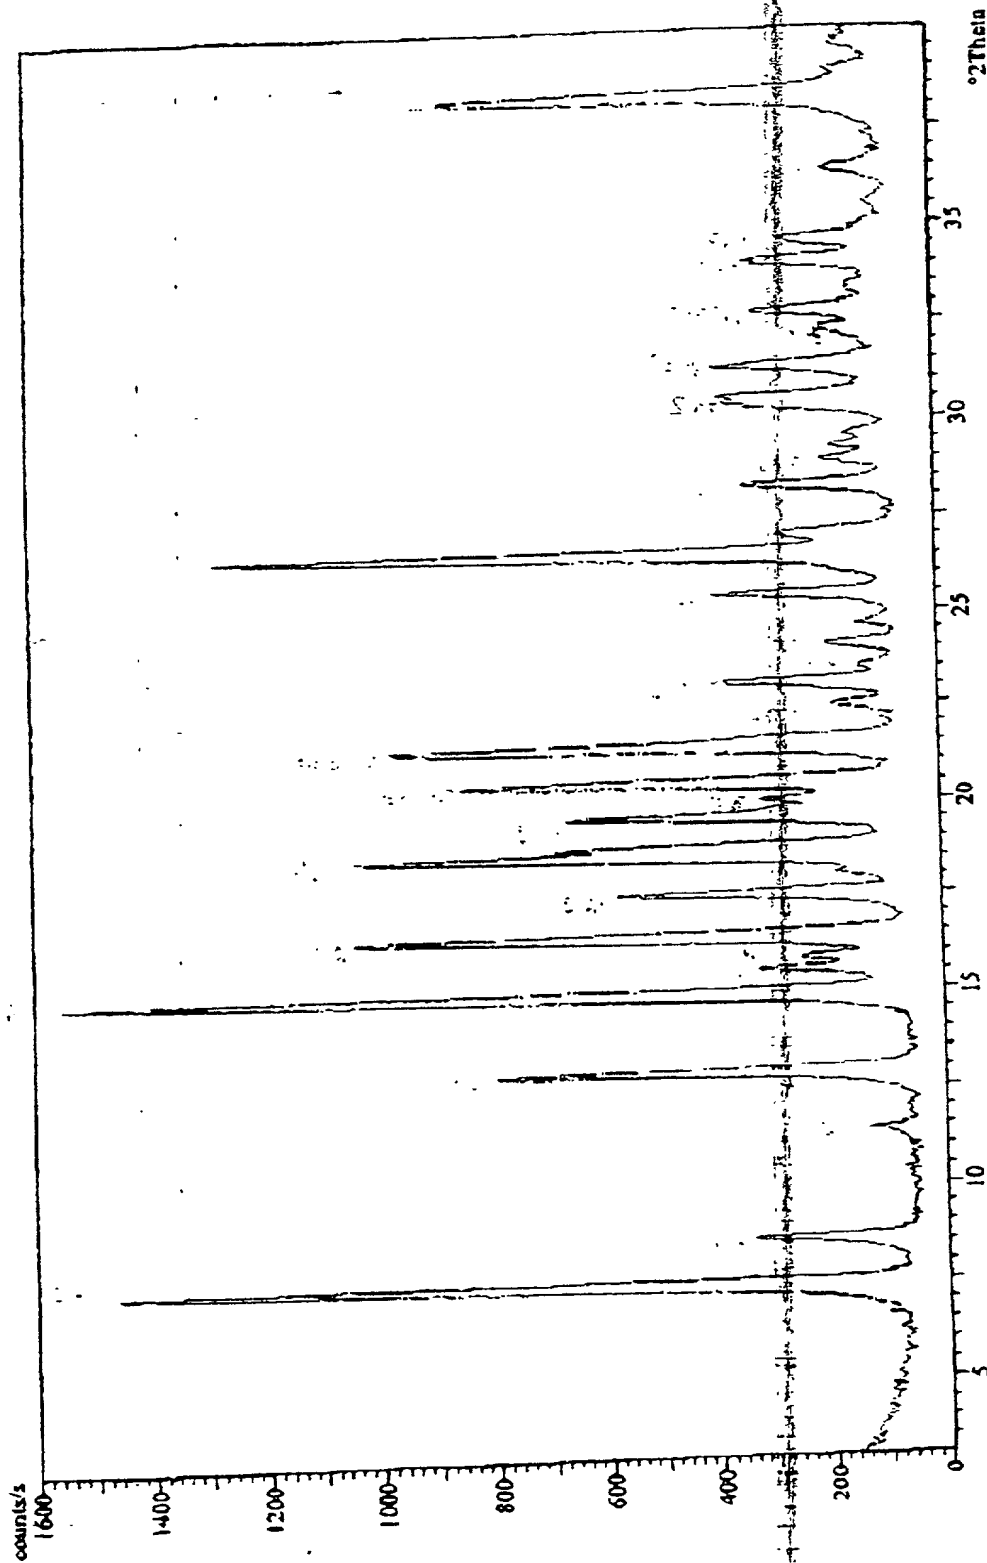


Figure 6

EXO

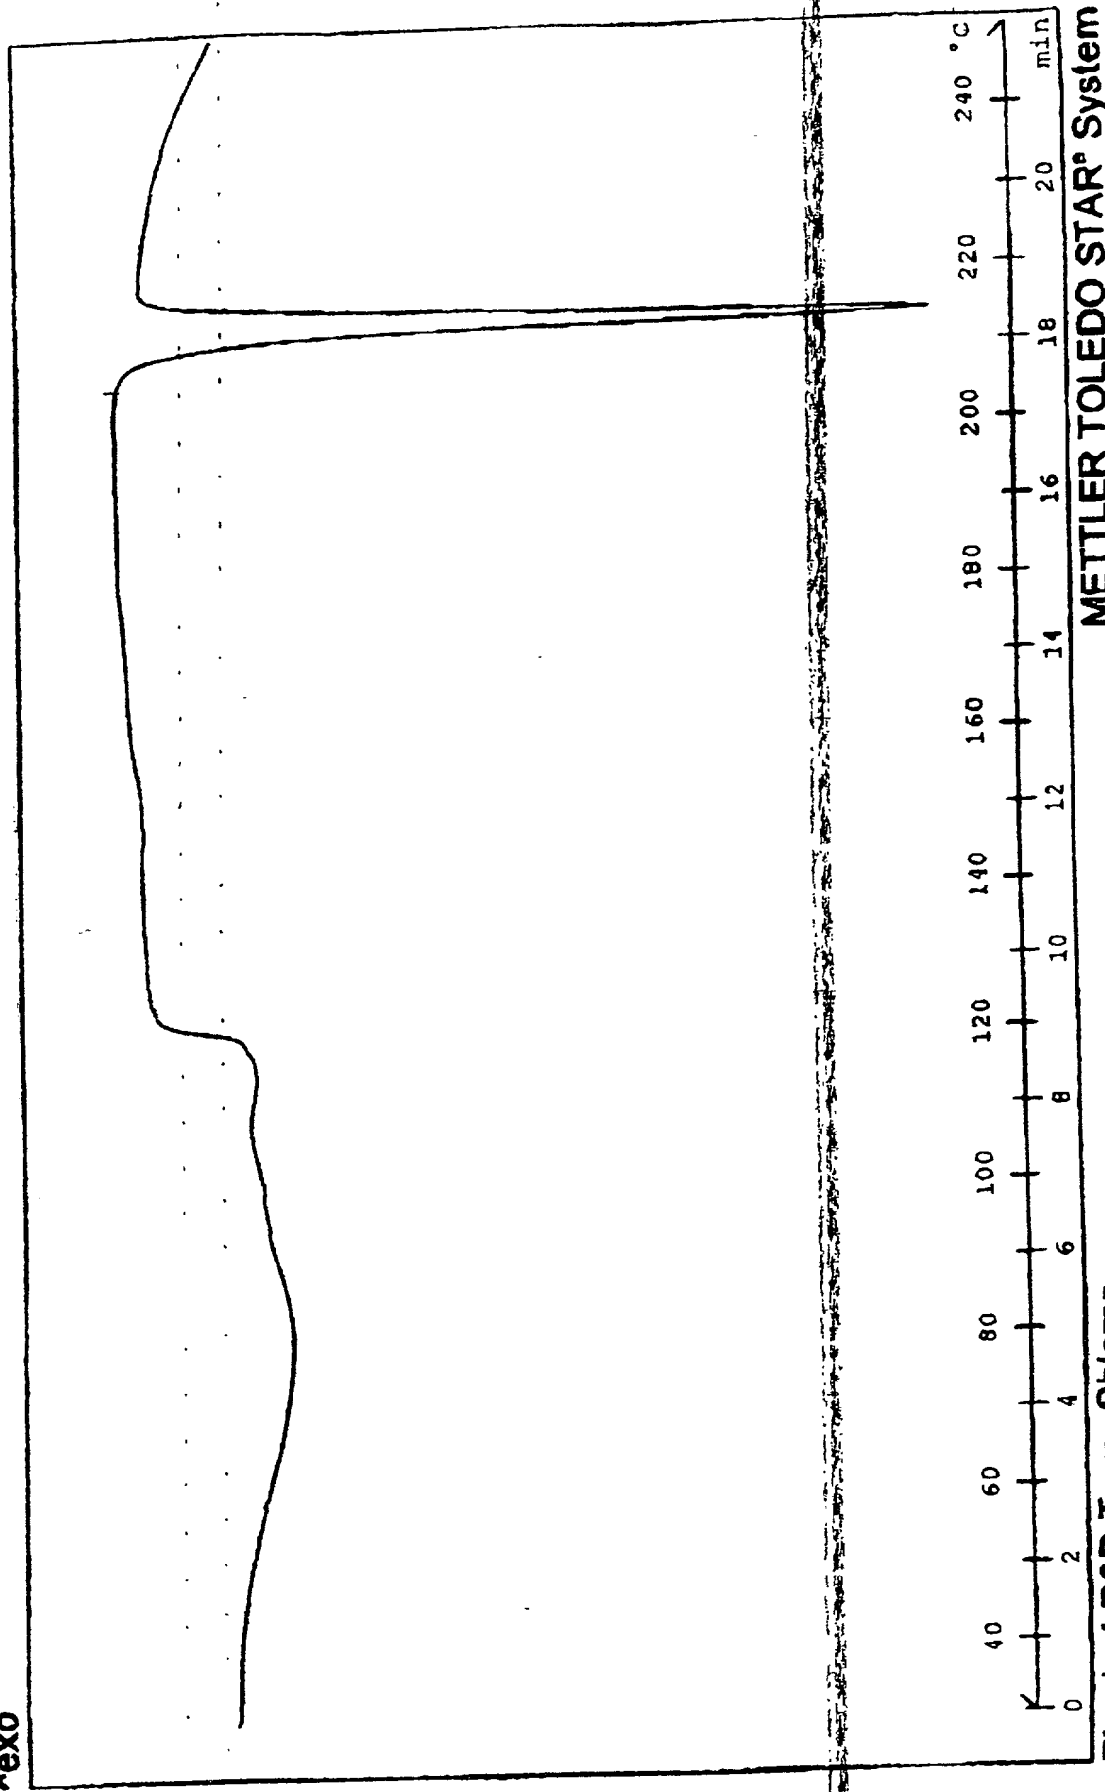

Physical R&D Teva: Shlomo

Figure 7

METTLER TOLEDO STAR® System

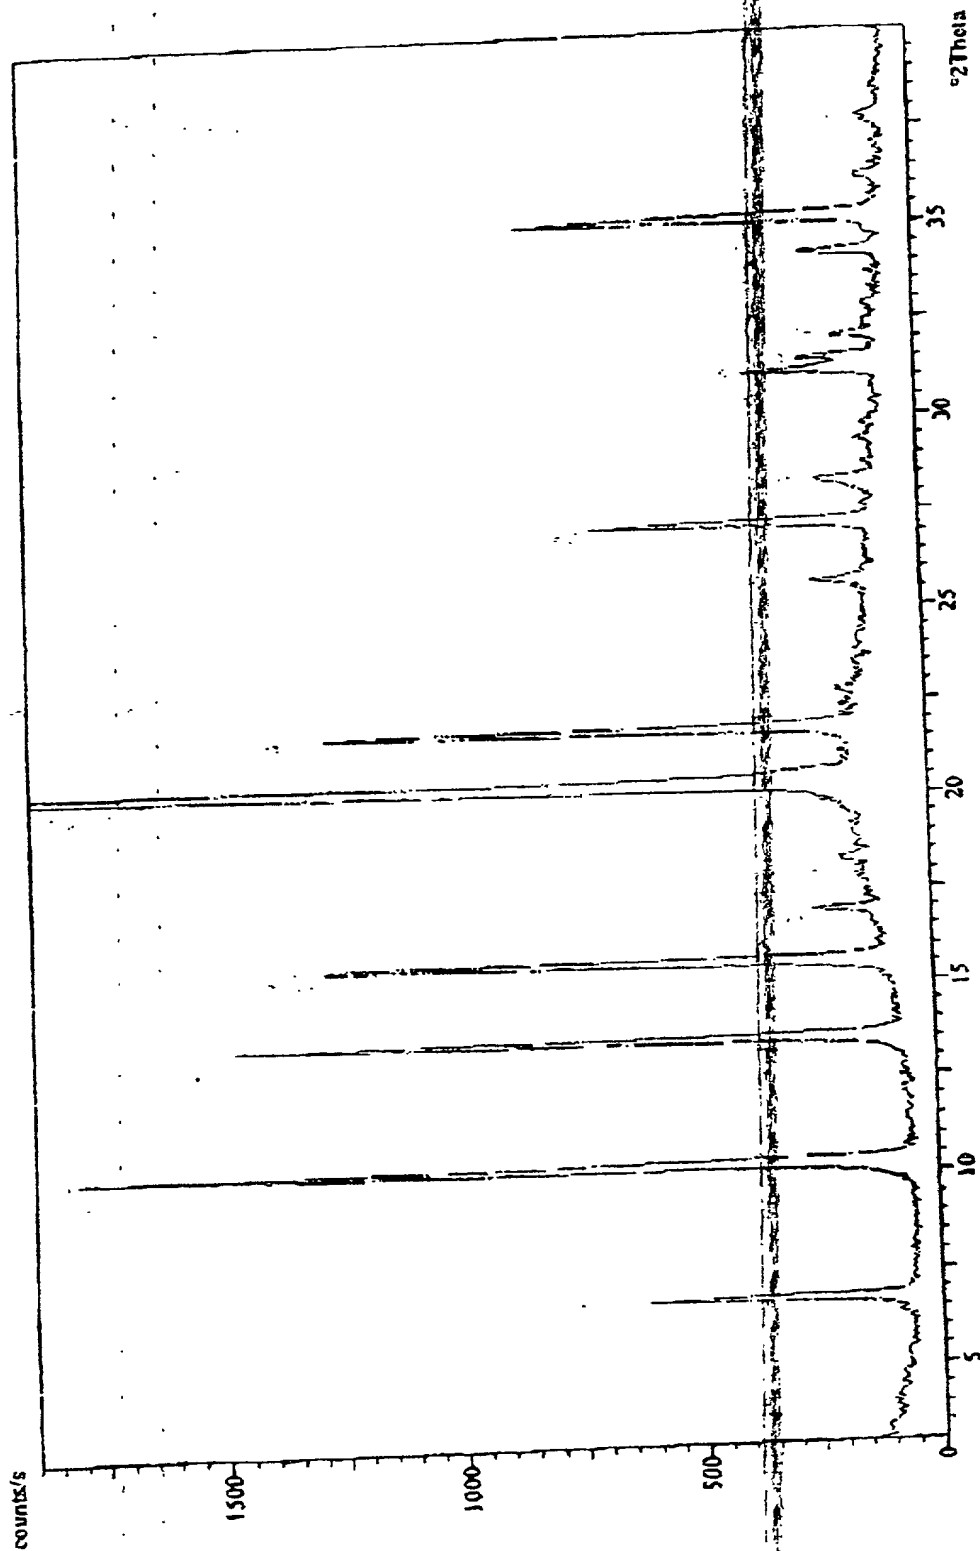


Figure 8



TOP OF SHEET

File: VEL-07 SHQ, ID: VEL-07 SHQ.  
Date: 02/01/01 13:16 Step: 0.050° Cnt Time: 1.000 Sec.  
Range: 2.00 - 40.00 (Deg) Cont. Scan Rate: 3.00 Deg/min. TEVA

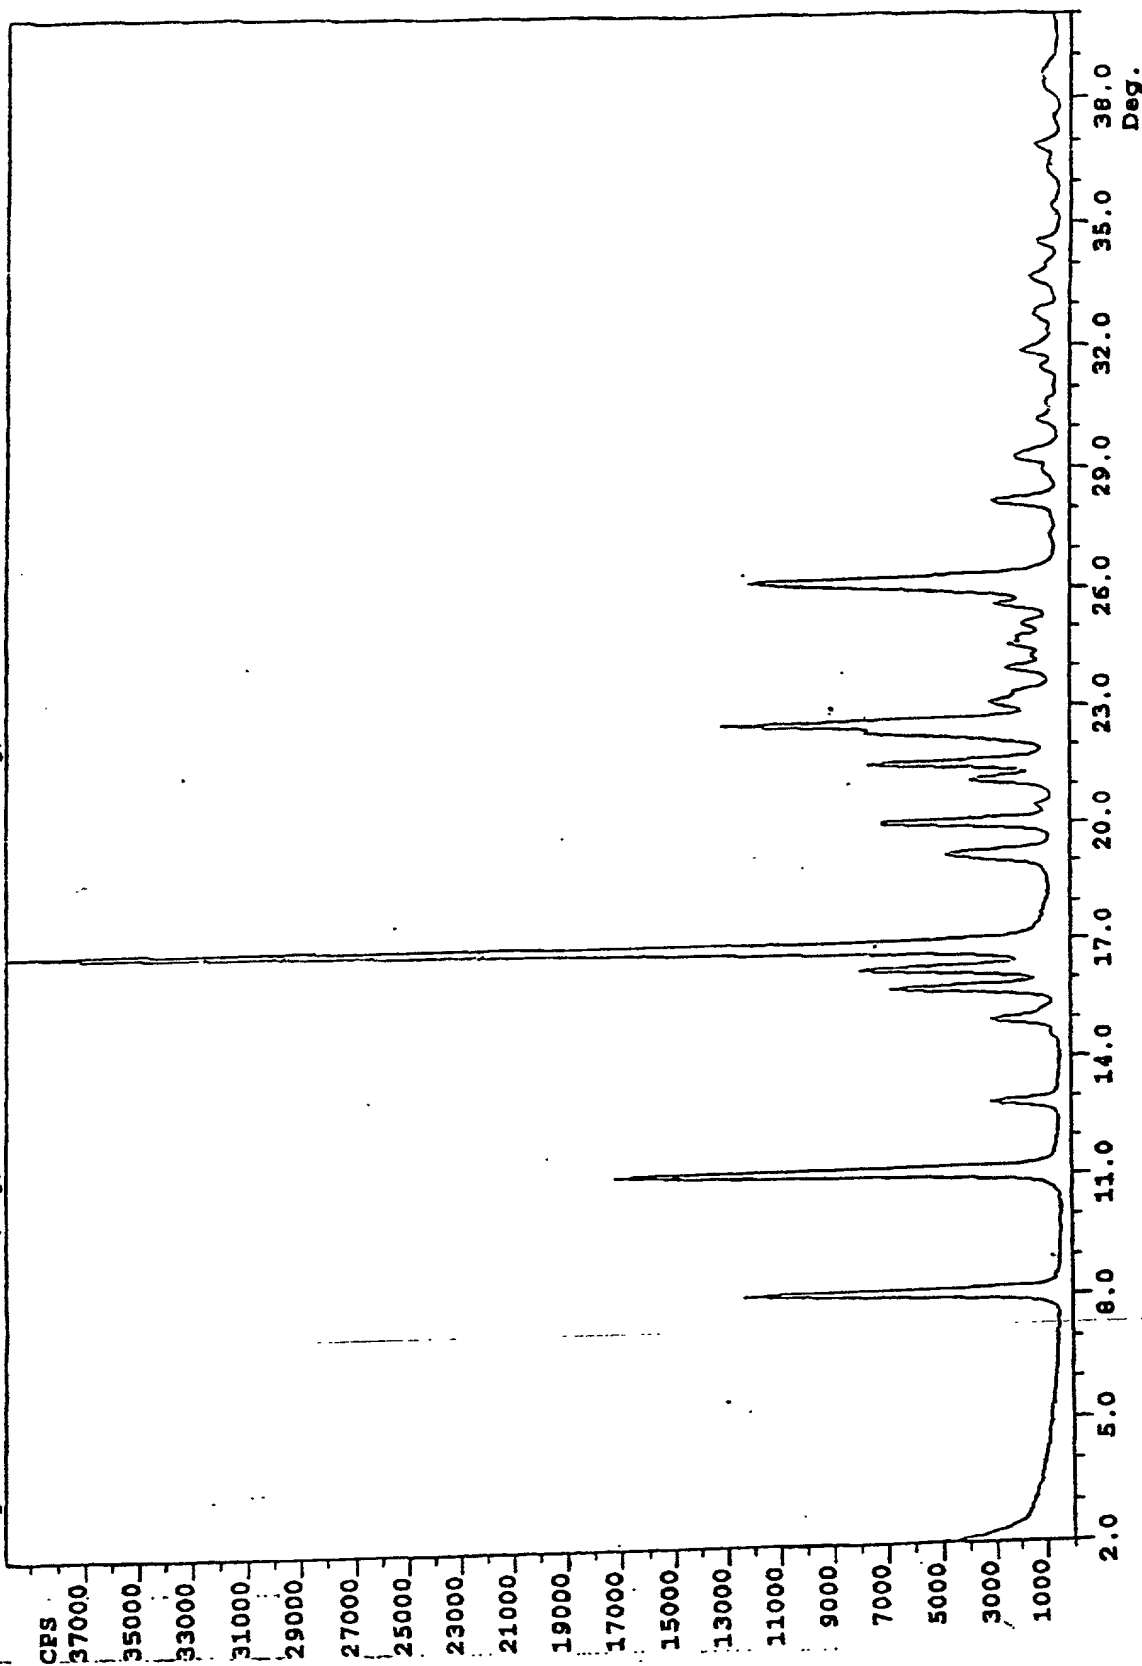


Figure 9

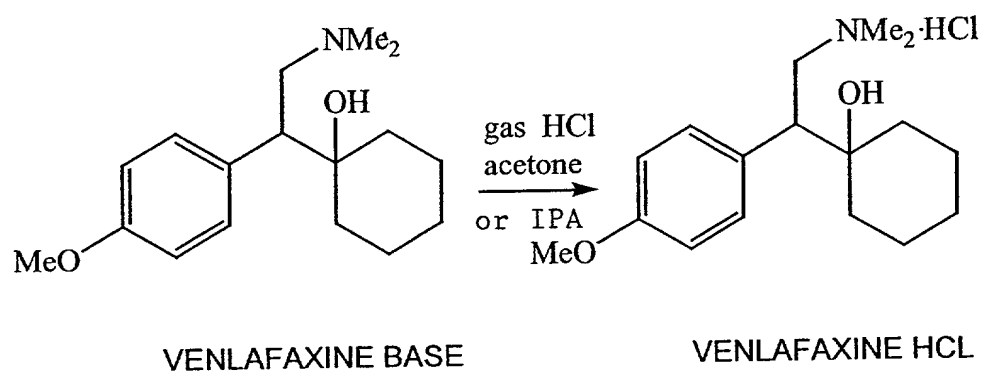


FIGURE 10